


EM=422

LCMS Scan ESI+

Ret. Time: 4.00

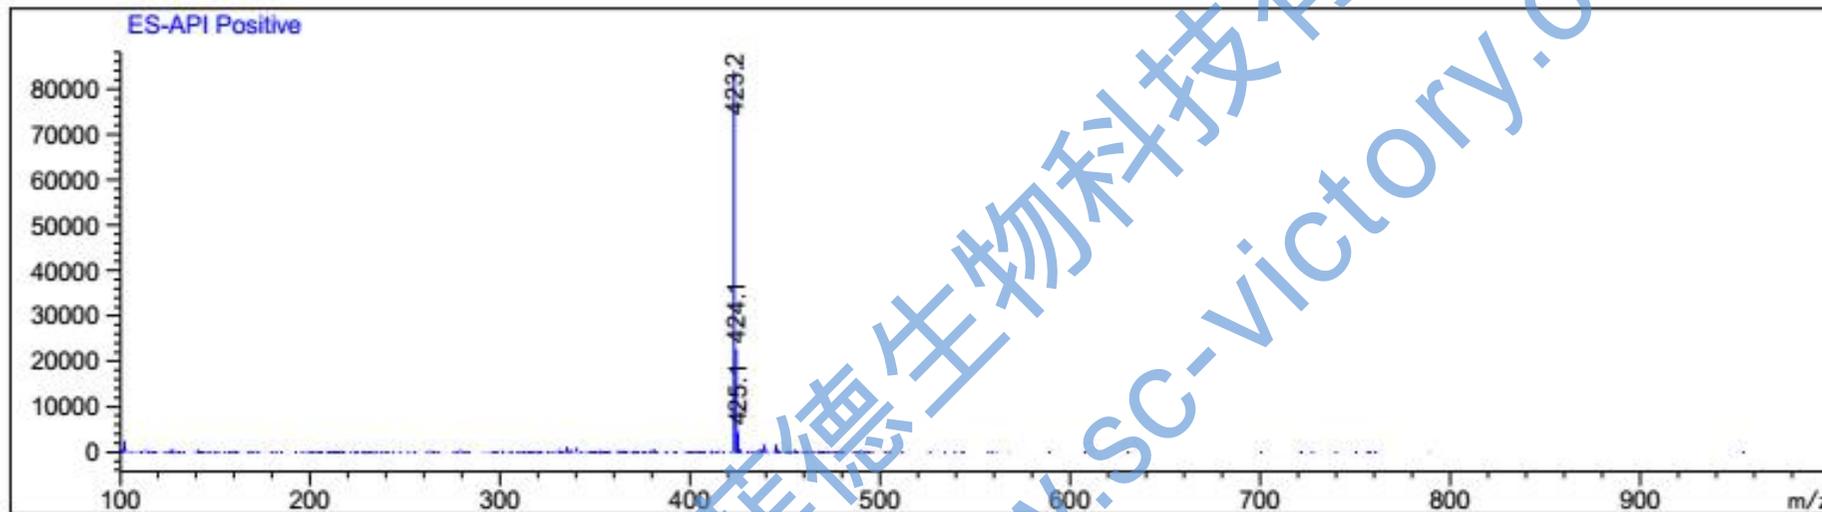


成都普菲德生物科技有限公司
<http://www.sc-victory.com>

EM=422

LCMS Scan ESI-

Ret. Time: 3.99

<<<< NEGATIVE SPECTRA >>>>

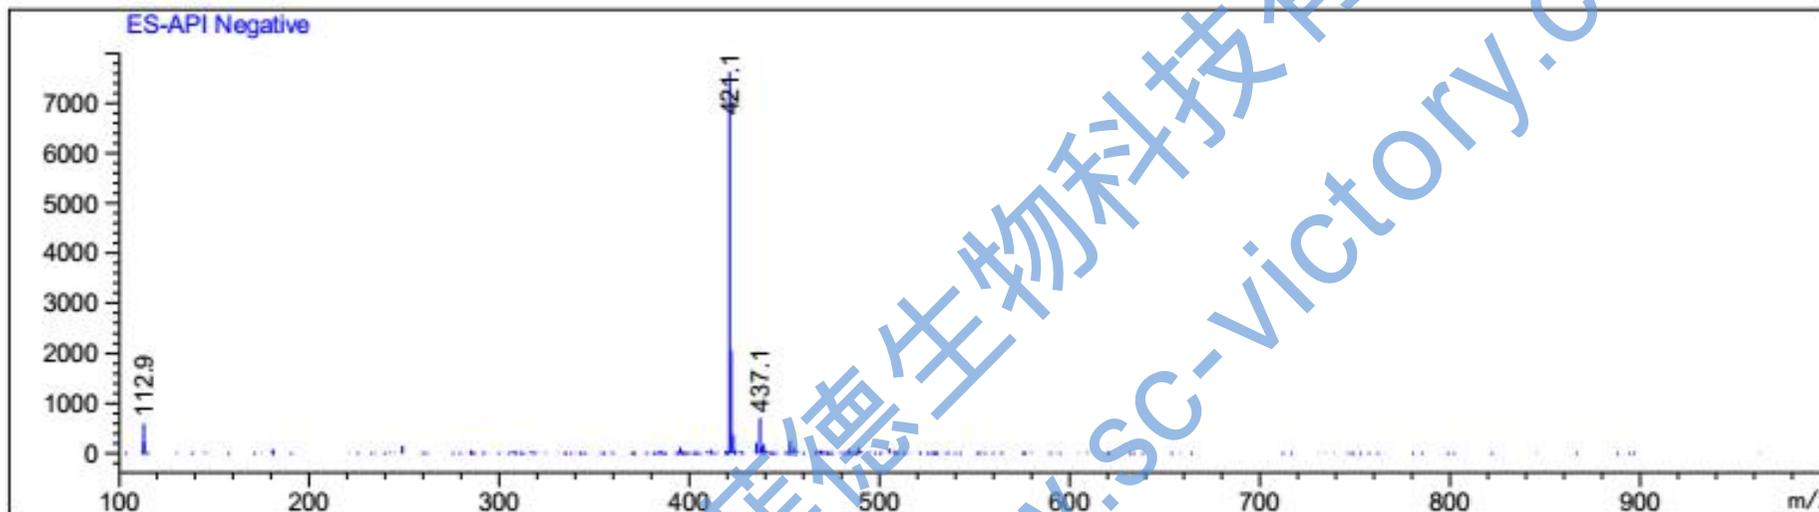

成都普菲德生物科技有限公司
<http://www.sc-victory.com>